



04-003B
2 May, 2007

FLOW DIRECTION OF A MOLY CONVERTER

I. PURPOSE:
To give information on the direction of flow through a Molybdenum converter

II. TOOLS:
None

III. PARTS:
None


IV. PROCEDURE:

This Service Note is to help you give you information on how to determine the flow direction of a Molybdenum converter.

Diagram 1 shows a TOP VIEW of the Molybdenum Converter cartridge. You will be able to tell which line on the cartridge is the Sample Inlet line by looking for the line that is at the center of the cartridge. The center line is always the Sample inlet. This is depicted in Diagram 1.

DIAGRAM 1

MOLY CONVERTER CARTRIDGE
TOP VIEW

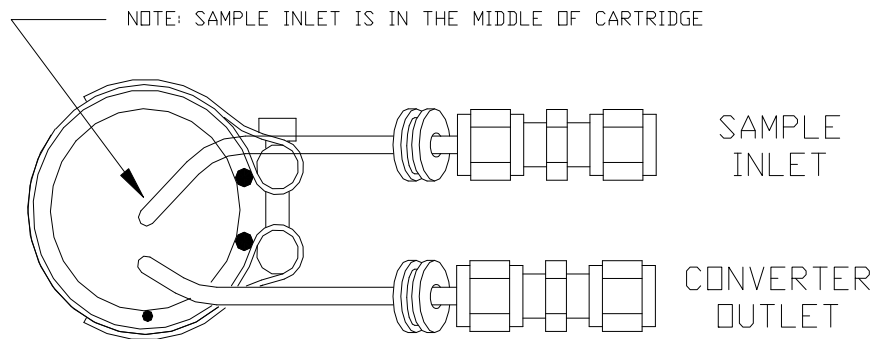

FLOW DIRECTION OF A MOLYBDENUM CONVERTER

04-003 Rev B

Page 1 of 3

Diagram 2 illustrates the connections of the Molybdenum Converter to the NO/NOX switching valve.

DIAGRAM 2

MOLY CONVERTER FRONT VIEW





Diagram 3 shows the pneumatic drawing of the M200A NOx Analyzer. The dashed line represents the sample flow through the instrument.

FLOW DIRECTION OF A MOLYBDENUM CONVERTER

04-003 Rev B

Page 2 of 3

DIAGRAM 3

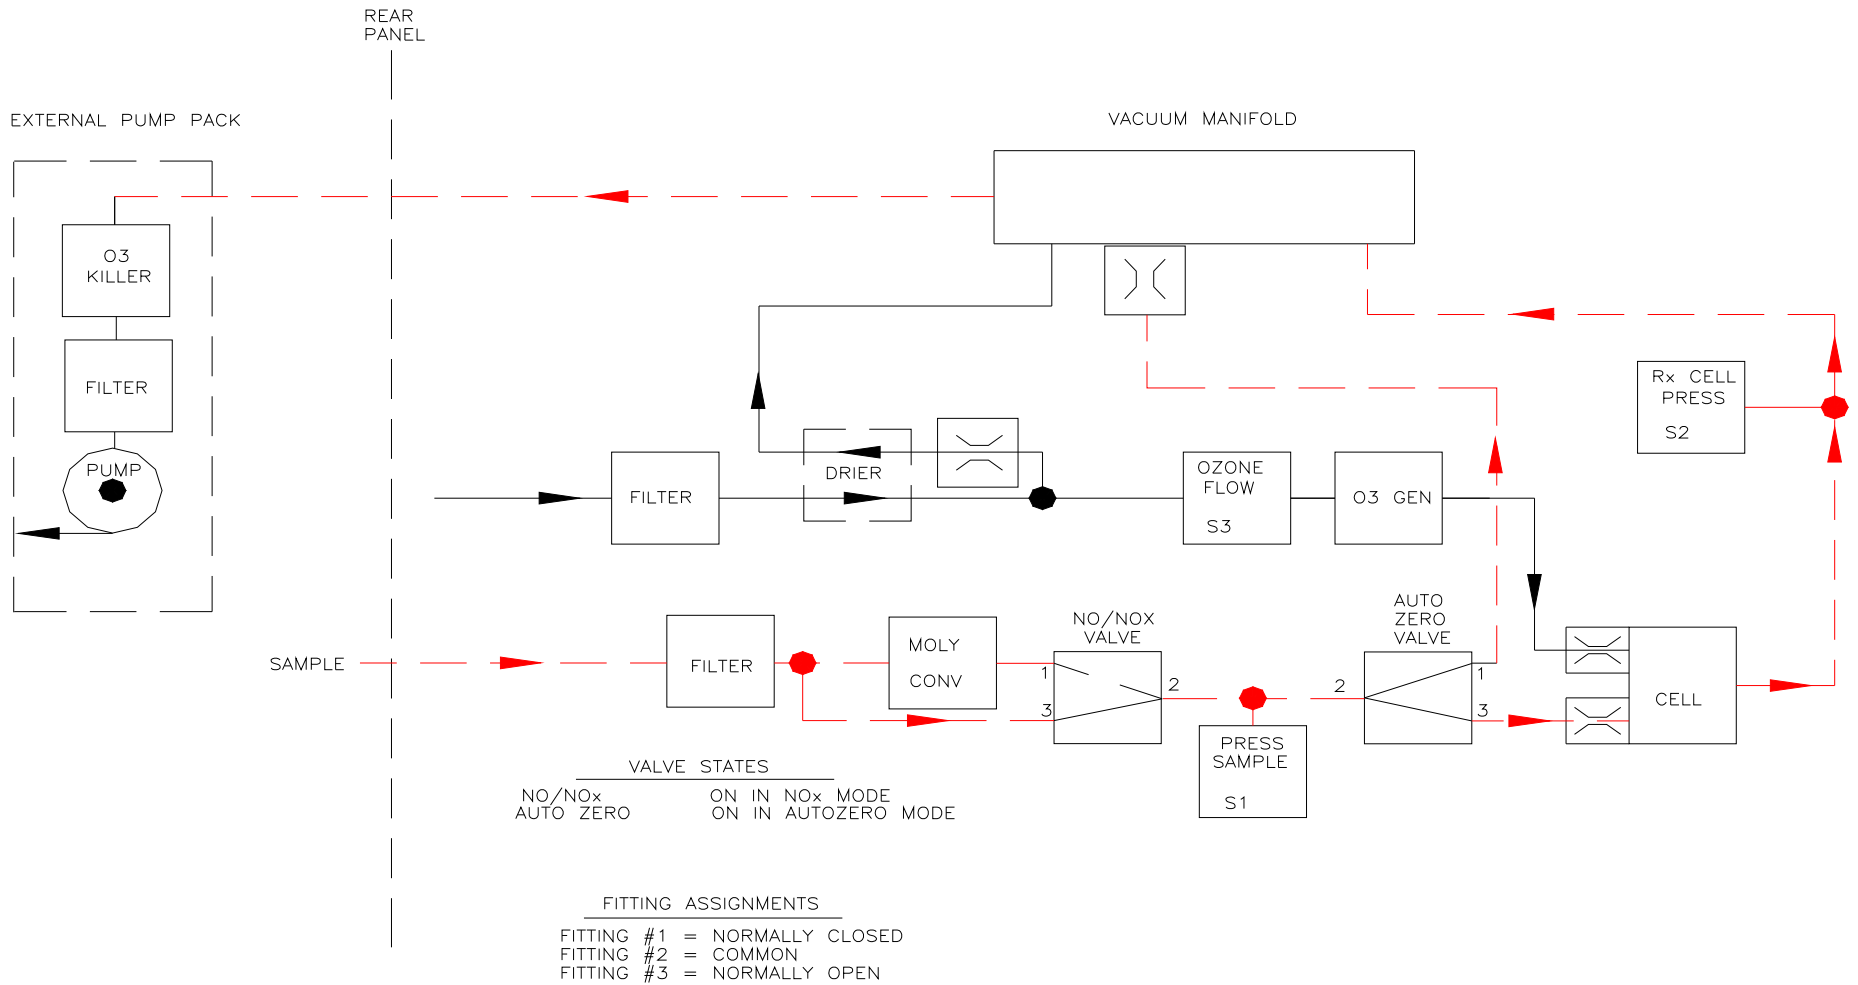

M200A PNEUMATIC DIAGRAM STANDARD CONFIGURATION

FLOW DIRECTION OF A MOLYBDENUM CONVERTER

04-003 Rev B

Page 3 of 3